

Cardiac Repolarization Analysis: Immediate Response

Josef Halamek¹, Pavel Jurak¹, Eleonora Tobaldini², Nicola Montano², Pavel Leinveber³

¹Institute of Scientific Instruments, Czech Academy of Sciences, Brno, Czech Republic

²Department of Biomedical and Clinical Sciences "L. Sacco", University of Milan, Milan, Italy

³St. Anne's University Hospital, ICRC, Brno, Czech Republic

Abstract

The reproducibility of QT parameters was tested on data recorded in subjects undergoing graded head-up tilt. Two QT detection algorithms were tested: D1 - on a beat to beat basis and D2 - on a 10-beats average basis. Relative irreproducibility, defined as $STD/mean$, in the case of D1 detection was 0.7, 6.3, 10 [%] for QT_c , QT/RR slope and QT restitution respectively. With D2 detection it was 0.7, 6.3, and 59 [%] respectively.

Conclusion: QT immediate response, i.e. the QT restitution, is reproducible parameter with D1 detection. D2 detection eliminates any information about QT restitution and does not increase the reproducibility of QT slow properties, as QT_c and QT/RR slope.

1. Introduction

Cardiac repolarization adaptation (represented by variation of QT intervals to RR changes) has two distinct phases: 1) an immediate response (restitution, i.e. the dependence on the preceding RR interval) and 2) a slow adaptation (memory, i.e. the dependence on amount of previous RR intervals). Both these phases are well known since many years ago. The time evolution of the action potential duration after sudden changes of cycle length has been measured by Franz [1]. Padrini [2] measured the adaptation of the QT interval to heart rate changes in an isolated, perfused guinea pig heart. The curve shapes presented by Padrini and Franz are similar. However, the analysis of restitution is mostly neglected, even if this parameter is significantly different between controls and Long-QT syndrome patients [3], it is modified by drugs such as dobutamine [4] and it is important in the analysis of fast short term QT variability. The reason for this lack of consideration is due to the low reproducibility of the measure, which can be related to inappropriate QT detection algorithm. Therefore, we tested the reproducibility of QT parameters using two different algorithms: a) D1 - on a beat to beat basis; b) D2 - on a 10-beats average basis, so called "global QT" [5].

2. Data

Analysis was performed on ECG signals recorded in three healthy volunteers during a graded head-up tilt protocol [6]. The subjects underwent six sessions, with tilt table angles randomly chosen (15, 30, 45, 60, 75, 90°). Each tilt session consisted in rest (7 min), tilt (10 min) and recovery (3 min).

Sampling frequency was 1000 Hz. The ECG lead with the best shape of T waves was used for the analysis. The RR and QT intervals were detected with our custom-designed software ScopeWin (Institute of Scientific Instruments, Brno, Czech Republic). The QT interval duration was determined from the onset of the QRS complex to the end of the T wave, defined as the crossing between the isoelectric line and the tangent to the descending T wave. The detection was visually checked and corrected (for RR intervals) or flagged as no detectable (for QT intervals).

The resulting RR and QT intervals series were used in the case of D1 detection. The moving window, with a length of 10 beats and an overlap of 5 beats, was used in the case of D2 detection. Median value of QT intervals from window was assigned to last QT interval from the window. QT intervals not assigned were set as not defined. The RR series were equal in both detections; QT series in case of D2 detection represent some type of "global QT" detection [5].

3. QT parameters

QT dynamic parameters are not yet standardized and they depend on supposed model of QT-RR coupling; different models have been used [7-12].

Our model is based on transfer function, defined by recursive relation (3 optimized parameters) between QT and RR intervals without mean levels [10, 11]. This model was given by Bayes optimization of the ARMA model, when the optimum between complexity and general parameter validity was analyzed [10]. The QT step response of this

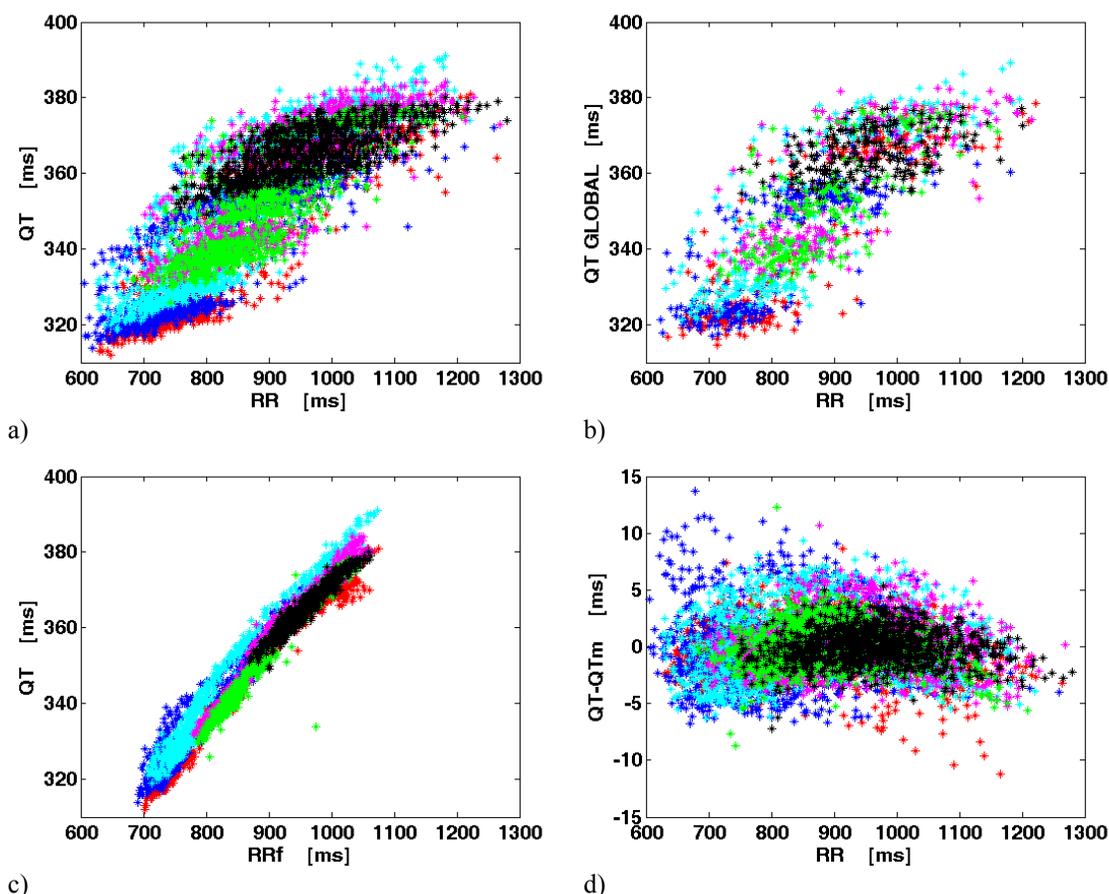


Figure 1. Subject S2, 6 tilt table angles. Order of plotting for different angles of tilt is: 90°, 75°, 60°, 45°, 30°, 15°, and corresponding colors are red, blue, cyan, magenta, and green, black. The successive plotting may overlap preceding plotting; i.e. only the measurement with 15° (black) is fully visible. a) D1 detection; b) D2 detection; c) QT hysteresis elimination according ARX model [11]; d) Error between detected QT (D1 detection) and predicted QT by model.

model, computed from optimized parameters, is always similar to a known QT step response measured in patients with pacemaker or in the isolated heart [1, 2]. This model defines the set of QT parameters for analyzed measurement: i) QTc, i.e., a 60-bpm equivalent QT duration computed from the QT/RR model; ii) the gain of QT-RR coupling for slow variability of RR (Gain_S), i.e., QT/RR slope, i.e. the parameter that describes QT memory; iii) the gain of QT-RR coupling for fast variability of RR (Gain_F), i.e. restitution, i.e. the parameter that describes the immediate change of QT; iv) the time constant of QT adaptation to RR changes; v) random QT variability, i.e. QT variability not dependent on RR changes. The parameters are not affected by hysteresis because the ARX model controls for it [11].

4. Results

Graphical results of detected intervals, hysteresis elimination and error between detected QT and QT

assessed from model for subject S2 over different tilt table angles are shown in Fig. 1. Mean levels \pm STD over 6 angles of tilt for subjects S1 to S3 are reported in Tab. 1 and relative inaccuracy given as STD/mean is reported in Tab. 2. Parameter distribution over different tilt table angles is represented in Fig. 2.

Table 1. Mean levels \pm STD over 6 tilt table angles for subjects S1, S2 and S3 and QT detections D1 and D2.

subject/ detection	QTc [ms]	Gain_S $\times 10$	Gain_F $\times 100$
S1/D1	362 \pm 2	1.72 \pm 0.06	2.4 \pm 0.2
S1/D2	362 \pm 2	1.71 \pm 0.06	0.55 \pm 0.36
S2/D1	374 \pm 3	1.86 \pm 0.14	3.3 \pm 0.5
S2/D2	374 \pm 3	1.86 \pm 0.14	0.68 \pm 0.32
S3/D1	369 \pm 3	1.71 \pm 0.14	3.3 \pm 0.2
S3/D2	369 \pm 3	1.70 \pm 0.14	0.41 \pm 0.26

Table 2. Relative inaccuracy (STD/mean \times 100) for subjects S1 to S3 and mean inaccuracy over subjects for QT detections D1 and D2

	QTc [%]	Gain _S [%]	Gain _F [%]
S1/D1	0.62	3.3	8.2
S1/D2	0.63	3.4	65.3
S2/D1	0.74	7.3	14.7
S2/D2	0.73	7.3	46.6
S3/D1	0.73	8.2	7.2
S3/D2	0.74	8.0	64.1
mean/D1	0.7	6.3	10.0
mean/D2	0.7	6.3	58.7

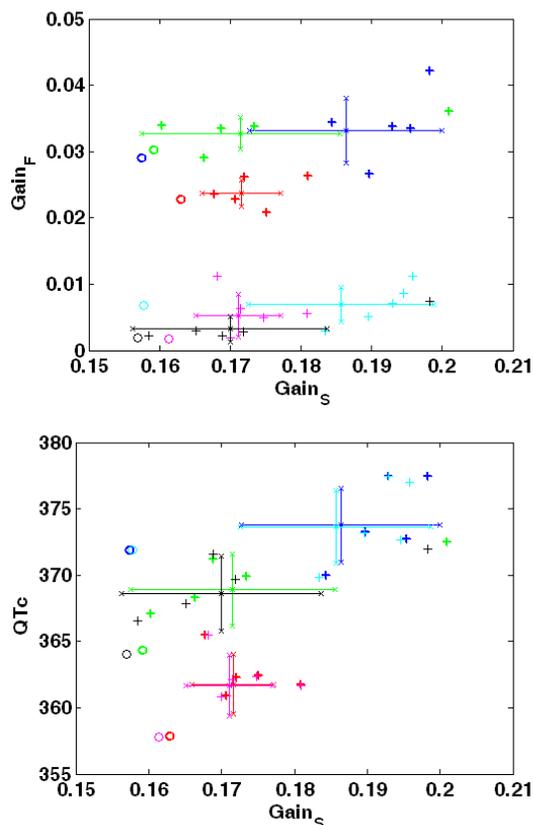


Figure 2. Parameters distribution. Crossing of lines defines mean and lines represent STD for given subject. Marks describe single measurement; 'o' represents tilt with angle 15. Colors define subject and detection. D1 detection: red, blue and green for subject S1, S2 and S3 respectively. With D2 detection corresponding colors are magenta, cyan and black.

5. Theory

D2 detection, based on averaging of ECG or detected QT intervals over few beats is the low pass filter. The fast QT variability is filtered out by this filter. The analyzed

frequency responses of QT-RR coupling with D1 detection and D2, together with influence of low pass filter on frequency response with D1 detection are in Fig. 3.

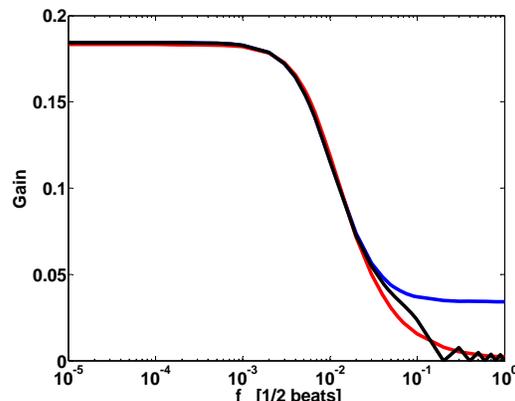


Figure 3. Analyzed frequency responses of QT-RR coupling with D1 detection (blue), D2 (red) and the influence of the low pass filter on response with D1 (black). Order of plotting: blue, red, black. Subject S2, angle 90°.

6. Discussion

The best reproducibility from tested QT parameters is at QTc (inaccuracy 0.7 %). The reproducibility of Gain_S and Gain_F is about order worse but acceptable. Inaccuracy is 6.3 and 10 % respectively.

Gain_F may be analyzed with QT detection beat per beat only. Using D2 detection ("global QT") the Gain_F cannot be analyzed. Averaging ECG signal or detected QT intervals over few beats eliminates fast QT variability and any information about Gain_F is missing (see Fig. 3). However, with D2 detection we cannot speak about reproducibility of Gain_F, as such parameter does not exist in analyzed data (see black line in Fig. 3). On the other hand, slow QT parameters (QTc and Gain_S) are not affected by type of QT detection (Fig. 2, 3, Tab. 1, 2).

According to our opinion, global QT and D2 detection should not be used anymore. They do not increase the accuracy of slow QT parameters and they eliminate the information about fast QT variability and about fast coupling between QT-RR.

The reproducibility of any parameter depends on signal-to-noise ratio (SNR) of analyzed data. SNR is given by ratio of QT variability corresponding to RR changes and QT variability not determined by RR changes (random QT variability and detection errors). With small RR changes, the majority of variability in detected QT intervals may be related to detections errors and random QT variability and so the minimal SNR of analyzed data is in measurements with tilt table angle of 15°. QT parameters from these measurements have

maximal differences from mean levels (see Fig. 2). Analyzing the reproducibility excluding the 15° angle, the inaccuracy of QT parameters decreased (data not presented).

In the analysis we suppose that QT parameters do not depend on angle of tilt. There may be some physiological dependency, as in [6] and QT parameters depend on excitation [13, 14]. In any case, SNR somehow depend on input data (angle 15°). The value of reproducibility may be increased by longer measurements or/and by increasing RR changes. The presented irreproducibility can be considered maximal, however significantly better reproducibility may be achieved.

7. Conclusion

QT restitution is a reproducible parameter and its analysis may be important in evaluating the prevalence of arrhythmias. This parameter may be analyzed with QT detection beat per beat only. Using global QT, i.e. averaging ECG per few beats, eliminates any information about restitution and such detection is probably the origin of the reported irreproducibility of restitution. Global QT has no contribution in accuracy of slow QT properties (QTc, QT/RR slope) and shouldn't be used anymore.

The reproducibility of QT parameters depends on SNR of analyzed data and the SNR may be increased by longer measurement and increased RR interval changes.

It is time to open more detailed discussion about QT detection, best QT/RR model and best set of QT parameters.

Acknowledgements

This work was partially supported by grant No. P102/12/2034 of the Grant Agency of the Czech Republic and by European Regional Development Fund – Project FNUSA-ICRC No. CZ.1.05/1.1.00/02.0123.

References

[1] Franz MR, Swerdlow CD, Liem LB, et al. Cycle length dependence of human action potential duration in vivo. Effects of single extrastimuli, sudden sustained rate acceleration and deceleration, and different steady-state frequencies. *J. of Clinical Investigation* 1988; 82: 972–979.

[2] Padrini R, Speranza G, Nollo, G. Adaptation of the QT interval to heart rate changes in isolated perfused guinea pig heart: influence of amiodarone and D-sotalol. *Pharmacological Research* 1997; 35: 409–416.

[3] Halamek J, Couderc JP, Jurak P, et al. Measure of the QT–RR Dynamic Coupling in Patients with the Long QT Syndrome. *Annals of Noninvasive Electrocardiology* 2012; 17:323–330.

[4] Seethala S, Shusterman V, Saba S, et al. Effect of β -adrenergic stimulation on QT interval accommodation. *Heart Rhythm* 2011; 8:264-270.

[5] Kligfield P. Electrocardiography and repolarization abnormalities in cardiac safety: benefits and limitations of fully automated methods for QT measurement. *Computing in Cardiology* 2010; 37: 253–256.

[6] Porta A, Gneccchi-Ruscione T, Tobaldini E, et al. Progressive decrease of heart period variability entropy-based complexity during graded head-up tilt. *J Appl Physiol* 103: 1143–1149, 2007

[7] Pueyo E, Smetana P, Caminal P, et al. Characterization of QT interval adaptation to RR interval changes and its use as a risk-stratifier of arrhythmic mortality in amiodarone-treated survivors of acute myocardial infarction. *IEEE Transaction on biomedical engineering* 2004; 51: 1511-1520.

[8] Razak E, Buncova M, Shusterman V, et al. Slow QT Interval adaptation to heart rate changes in normal ambulatory subjects. *Annals of Noninvasive Electrocardiology* 2011; 16: 148-155

[9] Jacquemet V, Dube B, Knight R, et al. Evaluation of a subject-specific transfer-function-based nonlinear QT interval rate-correction method. *Physiological Measurement*. 2011; 6: 619-635

[10] Halamek J, Jurak P, Villa M, et al. Dynamic coupling between heart rate and ventricular repolarization. *Biomedizinische Technik, Biomedical engineering*, 2007; 52:255-263, 2007.

[11] Halamek J, Jurák P, Bunch T, et al. Use of a novel transfer function to reduce repolarization interval hysteresis. *Journal of interventional cardiac electrophysiology*. 2010; 29:23–32.

[12] Halamek J, Jurák P, Vondra V, Lipoldová J, Leinveber P, Plachy M, Frana P, et al. Dynamic properties of QT intervals. *Computers in Cardiology* 2009; 36:517-520.

[13] Halamek J, Jurak P, Vondra V, et al. Excitation specificity of repolarization parameters. *IEEE Engineering in Medicine and Biology Society (EMBS) 2011*; 33:961-964.

[14] Paavonen KJ, Swan H, Piippo K, et al. Response of the QT interval to mental and physical stress in types LQT1 and LQT2 of the long QT syndrome. *Heart* 2001; 86: 39-44.

Address for correspondence.

Josef Halamek
Institute of Scientific Instruments, Czech Academy of Sciences
Kralovopolska 147, Brno 612 64
Czech Republic
josef@isibrno.cz